


Comment 1

Comment 2

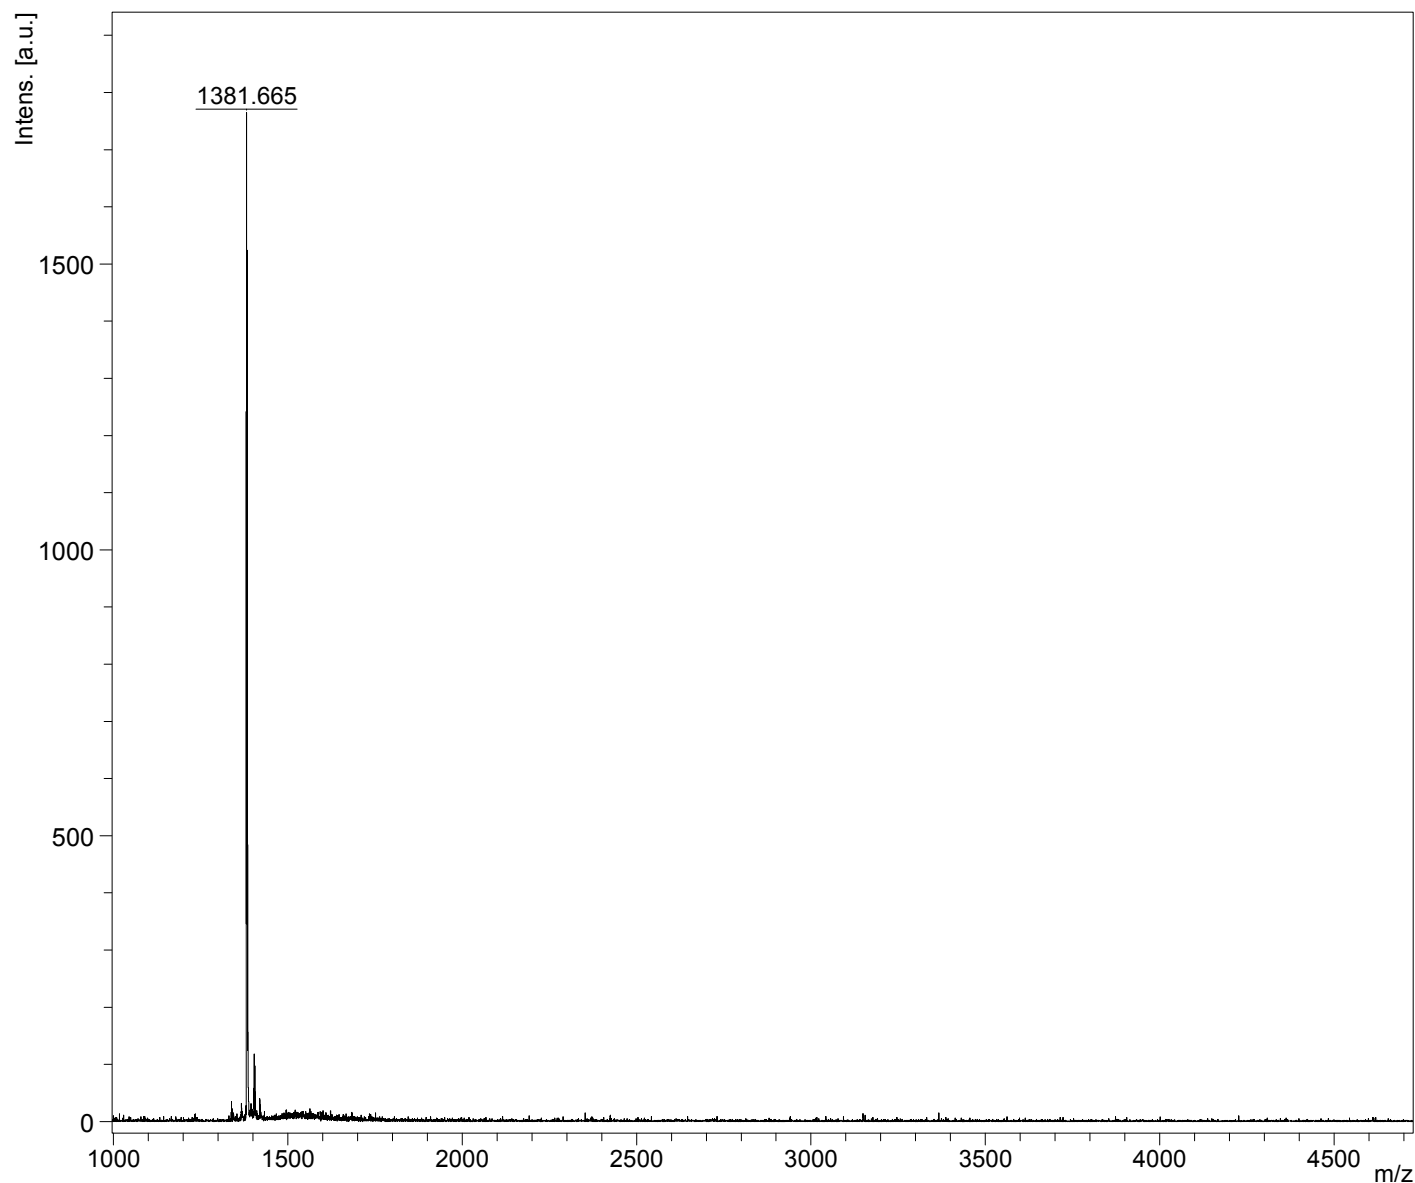

#### Acquisition Parameter

Date of acquisition	2023-02-14T12:26:38.921+01:00
Acquisition method name	D:\Methods\flexControlMethods\Regina\170712\RP_Proteomics_HPC.par
Spectrum type	TOF
Parent ion mass for ms/ms spectra	
Parent mass + PCIS upper mass limit	
Parent mass - PCIS lower mass limit	
CID valve/mode	

#### Instrument Info

User	RM
Instrument	PSYLABUFLEX
Instrument type	ultraflexTOF/TOF