


Comment 1

Comment 2

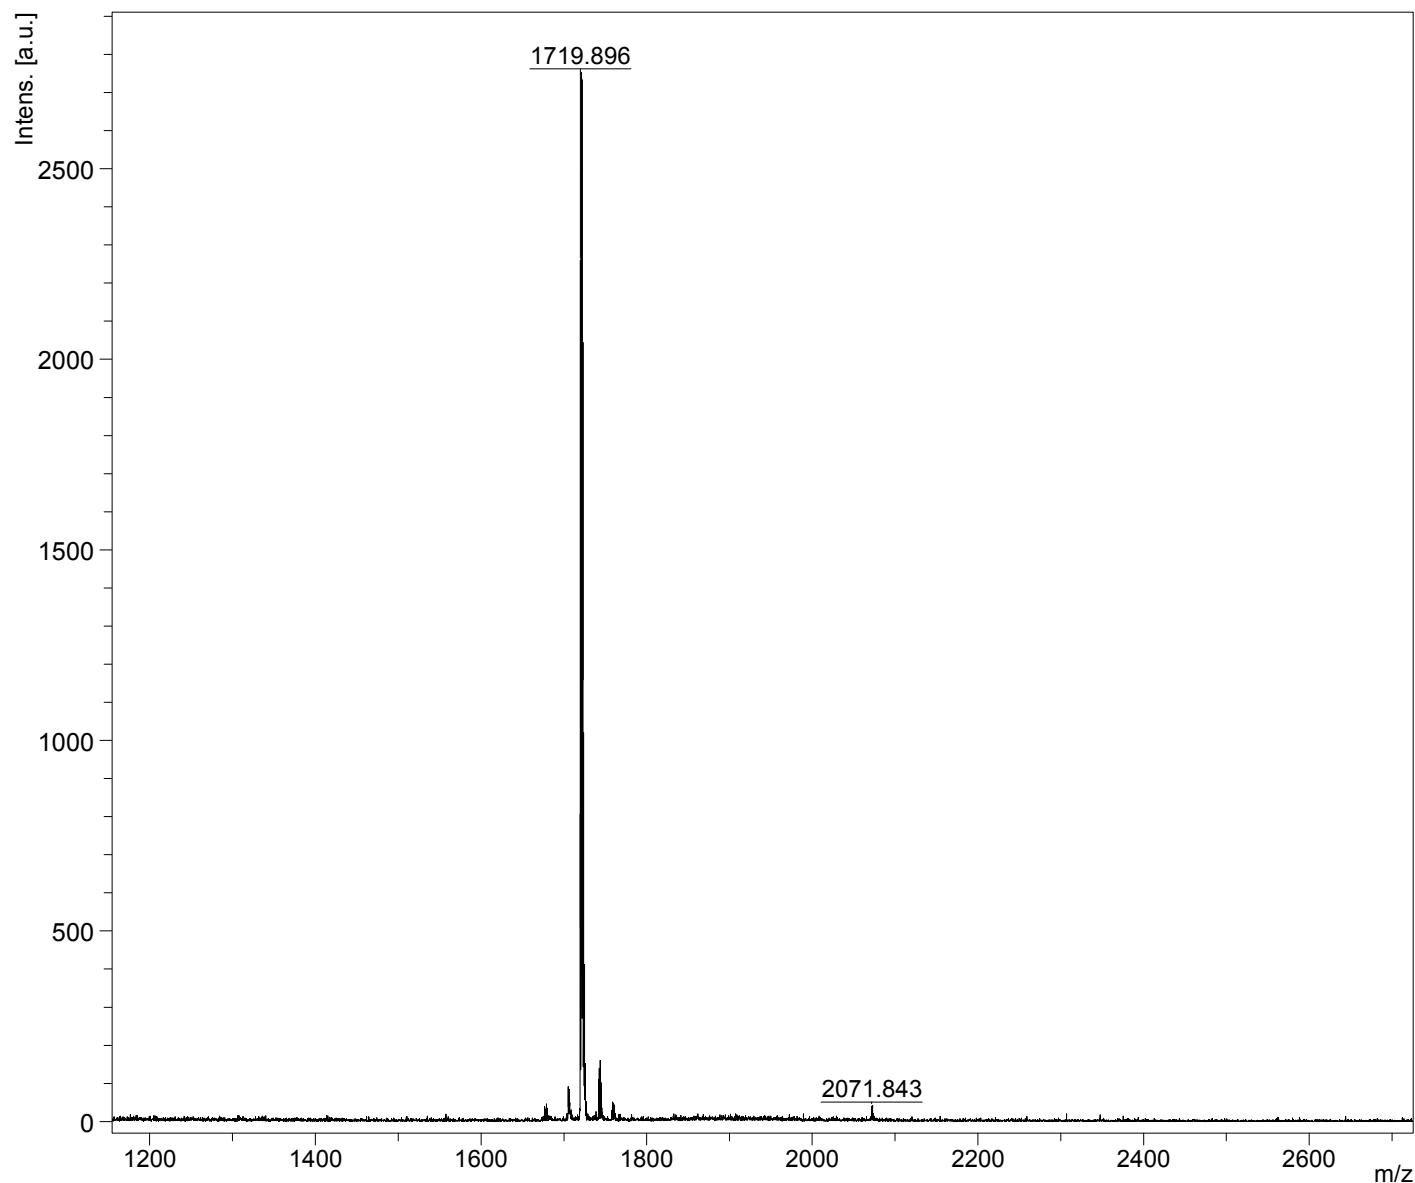

#### Acquisition Parameter

Date of acquisition 2023-02-14T12:28:05.328+01:00  
Acquisition method name D:\Methods\flexControlMethods\Regina\170712\RP\_Proteomics\_HPC.par  
Spectrum type TOF  
Parent ion mass for ms/ms spectra  
Parent mass + PCIS upper mass limit  
Parent mass - PCIS lower mass limit  
CID valve/mode

#### Instrument Info

User RM  
Instrument PSYLABUFLEX  
Instrument type ultraflexTOF/TOF